

WT3000-1FA Micro Gear Pump Drive Operating Manual

T3000-1FA



Baoding Longer Precision Pump Co., Ltd.



Baoding Longer Precision Pump Co., Ltd.

Building A, Chuangye Center, Baoding National High-Tech Industrial Development Zone Baoding, Hebei, China 071051

TEL: 86-312-3110087 FAX: 86-312-3168553

E-mail: longer@longerpump.com Http://www.longerpump.com





Important Information:

Please read operating manual carefully before operation.

- To prevent damage to pump, do not run the pump dry.
- If the power line or the plug are worn or damaged please pull out the plug (Hold the plug not the power line when pulling out).
- Please shut down the power supply and pull out the plug when you think the pump needs to be maintained or repaired.
- Shut down the power supply of the pump when connecting to external control equipment.
- The International Protection rating of this pump is IP31. Do not let liquid enter this pump drive.

Warranty:

- The warranty period of this product is one year. If repair or adjustment is necessary within the warranty period, the problem will be corrected at no charge if it is not due to misuse or abuse on your part, as determined by the manufacturer. Repair costs out side the warranty period, or those resulting from product misuse or abuse, may be invoiced to you.
- Contact Longer Company or Longer's dealers before returning pump to repair.
- Adopt original carton or reliable package when returning pump to repair.
- Write a note on detailed description of failure phenomena and contact information and put this note along with pump before returning pump to repair.




Micro Gear Pump Drive Operating Manual

Table of Contents

Instruction	1
Operating Panel	2
Basic Operation	2
Working Interface	3
Menu Navigation Diagram	5
Pump Head Operation	5
Pump Head Installation	5
Pump Heads and Flow rates	5
Pump Head Setting	6
Flow Mode Operation	6
Enter Flow Mode	6
Flow Setting	6
Flow Calibration	6
Flow Mode Operation Procedure	7
Dispensing Mode Operation	7
Enter Dispensing Mode	7
Dispensing Volume	7
Copy No	8
Flow Setting	8
Pause Time	8
Dispensing Calibration	g
Dispensing Mode Operation Procedure	9
External Control	10
External Enable Setting	10
Analog Signal Control	10
Footswitch Control	11
Communication Control Mode	12
External Control Output	13
Maintenance	13
Technical Specifications	13

Instruction

WT3000-1FA micro gear pump has two kinds of work mode of flow mode and dispensing mode, it can deliver flow rates from 85.7 to 2571.4 ml/min and dispense volume from 0.1 ml to 999 liters. WT300-1FA adopts 128×32 LCD to display all kinds of information and parameters, it is suitable for deliver high temperature and high pressure liquid.

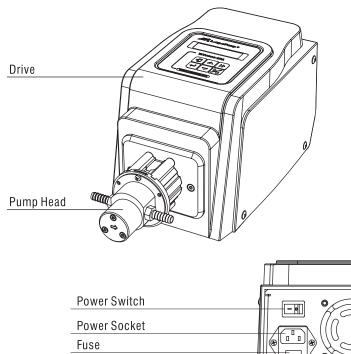


Fan External Control Output Interface External Control Input Interface

Reference:

Refer to page 10 to know the functions of External Control.

Operating Panel

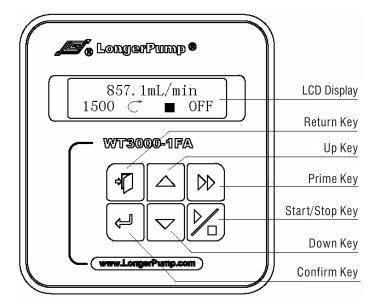

Basic Operation

Start/Stop Kev

Press Start/Stop key to stop or run the pump.

Prime Key

In flow mode, press **Prime Key**, pump will run at max. Speeds; in dispensing mode, press **Prime Key**, pump will run at max. speed to accomplish the operation of fast filling or fast emptying; press **Prime Key** again, the pump will return to previous state. In prime state, all the other keys are invalid.

Up Key/Down Key

Function 1: In flow mode, press **Up Key/Down Key** to adjust flowrates (it is invalid in priming mode).

Function 2: Mode selection function, press **Up Key/Down Key** to select submenu.

Function 3: Using for correcting, setting parameters and functions, such as dispensing volume, testing time, measured volume, copy No, footswitch, etc.



Confirm Key

Press **Confirm Key** to confirm the setting of entering menu, parameters selection.

Return Key


Function 1: Cancel current setting, return to previous menu.

Function 2: In dispensing mode, press Return Key to review the current speed and the time for dispensing a target volume.

Working Interface

- There is a option of Language Selection, users can select suitable language by pressing Up Key/Down Key after power on the pump.
- Display working interface after initializing the pump.

Flow rates display




Instruction

- a. Current flow rate: In non priming mode, press Up Key/Down Key to adjust the
- b.Current speed: Display current rpm, it will change when adjusting flow rates.
- c.Direction: Instructed the machine running direction, the direction could not be changed.
- d.Running status: 【▶】 means the pump runs; 【■】 means the pump stops; [>>] means the pump is in prime state.
- e.Control Mode: INT means the pump is controlled internally; V means the pump is controlled by external analog voltage signal; **mA** means the pump is controlled by external analog current signal; Hz means the pump is controlled by external 0 10 kHz pulse signal. Off means shutting off the external control function by setting menu.

Micro Gear Pump Drive Operating Manual


❖ Dispensing Display

Dispensing status can be displayed in two interfaces (see illustration below), these two interfaces can be switched by pressing Return Key.



- b.Current speed: Display current rpm, it will change when adjusting dispensing volume or flow rates.
- c.Direction: Instructed the machine running direction, the direction could not be changed.
- d.Running status: [] means the pump runs; [] means the pump stops; [>>] A.means the pump is in prime state.
- f.Dispensing volume: Display the dispensing volume.
- g.Copy: Display the copy number in dispensing mode.
- h.Dispensing time: Display the dispensing time. When the dispensing procedure starts, the dispensing time will be counted down. Adjust the flow rates or dispensing volume to change the dispensing time in dispensing parameters setting interface.

Menu Navigation Diagram

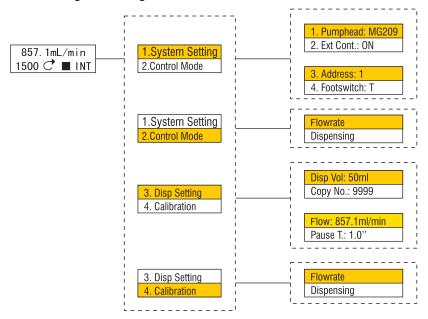

Pump Head Operation

Pump Head Installation

The pump head is mounted on drive before the pump leaves the factory. Follow below procedure for changing another pump head.


- 1.Loose the three M3 screws which connect the pump head and the pump head bracket. Dismantle the pump head slightly.
- 2.Put the new pump head in the old pump head location. Pay attention to the inlet and outlet locations of the pump head. Use three M3 screws to connect the pump head and the pump head bracket.
- $\widehat{\mathbb{V}}$ Turn off the power supply before changing the pump head.

Pump Heads and Flow rates

Acceptable Pump Heads	Product Code	Flow Rates (ml/min) 300-3000 (rpm)
MG204	05015010001	85.7 – 857.1 mL/min
MG209	05015010002	171.4 – 1714.3mL/min
MG213	05015010003	257.1 – 2571.4mL/min


Pump Head Setting

Press **Confirm Key** to enter Pump head interface, press Up Key or Down Key to select suitable pump head and then press **Confirm Key** to save the setting or press **Return Key** to cancel the setting and return to previous menu.



Flow Mode Operation


Enter Flow Mode: Press Control Mode to enter next interface, press Up Key or Down Key to select Flowrate, press Confirm Key to save or press Return Key to cancel the setting and return to previous menu.



Flow Setting: In Flowrate mode, press Up Key or Down Key to adjust the flow rates of pump.

❖ Flow Calibration

- See below diagram, enter Calibration interface, press Up Key or Down Key to set the
 testing time, the range of testing range is from 30 to 1800 seconds, press Confirm
 Key to save the setting or press Return Key to cancel the setting and back to
 previous menu after select a certain testing time value.
- The pump will display the running time and actual volume after pressing Start/Stop Key to start the calibration of pump. Running time will count down until testing time is over. Press Up Key or Down Key to input measured volume, press Confirm Key to save the setting. The calibration operation can be repeated.

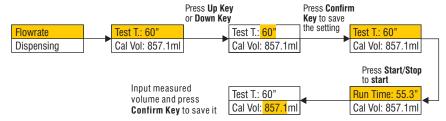




 If the actual volume is known in advance, enter the calibration interface and input the actual volume directly.




Flow Mode Operation Procedure

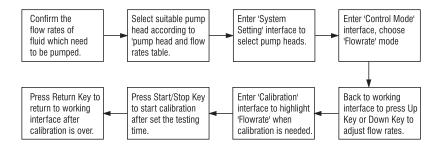


Dispensing Mode Operation

- $\widehat{\mathbb{Q}}$ It is recommended installing a one-way valve to prevent liquid reflux which will affect the accuracy of dispensing volume before starting dispensing mode.
- **Enter Dispensing Mode:** Press **Confirm Key** to enter Control Mode interface, press Up Key or Down Key to select work mode, press Confirm Key to save the setting or press **Return Key** to cancel the setting and return to previous interface.



- **Dispensing Volume:** The volume to be dispensed between two time intervals.
- Enter Dispensing Setting interface, press **Up Key** or **Down Key** to set dispensing volume. press **Confirm Key** to save the setting or press **Return Key** to cancel the setting and return to previous interface.
- Running time will be changed corresponding to the changing of dispensing volume.



Micro Gear Pump Drive Operating Manual


- **Copy No.:** The dispensing times are from 0 to 9999 times in Dispensing work mode.
- Enter Dispensing interface, press **Up Key** or **Down Key** to set the copy number, press Confirm Key to save the setting or press Return Key to cancel the setting and back to previous interface.
- If set Copy Number to Zero, dispensing cycles will be an infinite loop approach to work.



- * Flow Setting: The flow rates mean the flow rates in dispensing mode, the running time will be changed when adjusting the flow rates.
- Enter Flow rates interface, press **Up Key** or **Down Key** to set the flow rates, press **Confirm Key** to save the setting or press **Return Key** to cancel the setting and back to previous interface.




- * Pause Time: The Pause time between two dispensing cycles.
- Enter Pause Time interface, press Up Key or Down Key to set the pause time, press **Confirm Key** to save the setting or press **Return Key** to cancel the setting and back to the previous interface.







- * Dispensing Calibration: The parameters can not be changed under dispensing calibration, the default parameters are the parameters of dispensing mode.
- Enter Dispensing Calibration interface.
- Press **Start/Stop Key** to start the Calibration, and then enter next interface to display the Running Time and Measured Volume, the running time will count down until the calibration is over.



• If the measured volume is known in advance, user can input the measured volume directly using **Up Key** and **Down Key** in calibration interface. It is unnecessary to repeat above steps.




Dispensing Mode Operation Procedure

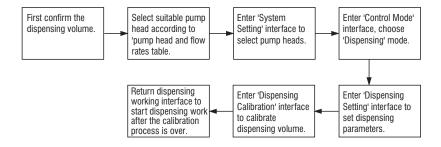

Micro Gear Pump Drive Operating Manual


External Control



❖ Analog Signal Control

Set 'Analog Signal Control' in enabling mode.

- Five kinds of external control module need to be ordered individually.
- Enter Flow rates interface, press **Up Key** or **Down Key** to set the flow rates, press **Confirm Key** to save the setting or press **Return Key** to cancel the setting and back to previous interface.



❖ External Control Enable Setting

Setting External Control Enable

Enter External Control Enable interface, press **Up Key** or **Down Key** to 'on' or 'off' the External Control, press Confirm Key to save the setting or press Return Key to cancel the setting and back to previous interface.



❖ Terminal Definition of External Control Module


- #1: Analog input in 4-20mA, 0.5-5V, 1.0-10V external control modules, control the speed of the pump. It is open in 1-10KHz external control module.
- #2: External control start/stop input. Open or input low level, the pump runs, Input high level, the pump stops.
- #3: Open

10

9



- #4: Analog ground in 4-20mA, 0.5-5V, 1.0-10V external control modules; Pulse input end in pulse input external control module, control the speed of the pump.
- **#5:** The COM of external control start/stop signal input; the COM of frequency input.

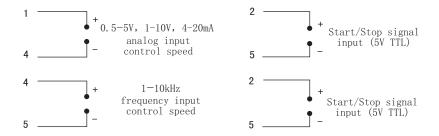


Footswitch Control

- Footswitch connect to external control interface to control the Start/Stop of pump. It can be set in menu according to actual requirement.
- · Footswitch has two kinds of work modes.

Trigger: Press footswitch, the pump starts running; press footswitch again, the pump stopes.

Gated: The pump runs as long as the footswitch is pressed.

See below diagram, enter 'Footswitch' interface, press **Up Key** or **Down Key** to select suitable work mode, press **Up Key** or **Down Key** to select suitable work mode, press Confirm Key to save the setting or press Return Key to cancel the setting and back to previous interface.



- Pump can automatically identify footswitch when a footswitch connected with a pump, in the meantime Start/Stop Key will be invalid. This status doesn't have any relation with external control enable setting.
- Footswitch need to be ordered individually. The suitable footswitch for this pump is JK-3.

Micro Gear Pump Drive Operating Manual


Communication Control Mode

- This pump can connect with upper computer (Computer, SCM, PLC) through RS485 serial communication module. Please contact Longer Company for communication protocol.
- Address Setting

A single upper computer can control up to 30 pumps when pumps are controlled by upper computer through RS485. Each pump must be assigned an individual address.

Set the address

See below diagram, Enter 'pump ID' interface, press Up Key or Down Key to set pump ID (1-30), press **Confirm Key** or press **Return Key** to cancel the setting and back to previous interface.



❖ External Control Output

Pump is equipped with output port in order to monitor the status of pump. Output signal adopts optoelectronic isolation circuit. A pull-up resistor and power supply are needed when using.

Terminals definition:

DB9-1: Start/Stop output, pump outputs low level when pump runs; pump outputs high level when pumps stops.

DB9-8: Frequency output, 300-3000 rpm corresponding to 1.25-12.5 KHz.

DB9-4,6,7: COM

Maintenance

The pump head and the surface of drive don't have chemical resistance to organic solution and high corrosive liquid, so the pump head and the surface of drive should be keep dry and clean or pump life will be shortened.



Technical Specifications

❖ Main Functions

Suitable Pump Heads	MG204, MG209, MG213
Operating Mode	Membrane keypad to set parameters and control the pump
Prime Function	Fast filling, cleaning and emptying
Display Function	128×32 LCD display all the information
External Control Input	Control flow rates and start/stop of the pump in flow mode
Footswitch	Control the start/stop of pump
External Control Output	Output the signals of Start/Stop and speed
Communication	Communicate with upper machine or computer
Flow Function	Deliver fluid as set flow rates
Dispensing Function	Set dispensing volume, copy number and pause time, etc
Memory Function	Store all the running information automatically
Calibration Function	Acquire higher accuracy
Cooling Function	Heat-emitting fan
Direction	Clockwise only

13

Specifications

Flow	Rates	85.7 to 2571.4 ml/min		
Dispe	nsing Volume	0.1ml to 999 liters		
Сору	No.	0-9999, zero means infinite cycle		
Pause	e Time	1 second to 999 hours, resolution is 0.1 second		
Flow Rate Calibration		30 seconds to 30 minutes, resolution is 1 second		
trol	Input Function	4-20mA, 0.5-5V and 1.0-10V modules control flow rates, TTL control the Start/Stop of the pump		
External Control	Output Function	Output the status of Start/Stop and 1.25-12.5kHz corresponding to 300-3000 rpm under the optical isolation mode		
	Communication	RS485		
Liqu	id to be pumped	The diameter of particle in liquid is smaller than 10µm		
Acceptable Liquid Temperature		PTFE: -45-50°C, PEEK:-45-120°C		
Mavin	num Outlet Pressure	MG204: 1.4MPa		
	ng Medium: Water)	MG209: 0.9MPa		
(16311	ilg Mediuiii. Water)	MG213: 0.8MPa		
Accep	table Liquid Viscosity	≤200cst		
Power	Supply	AC220V or AC110V, 50Hz/60Hz		
Power Consumption		≪50W		
Operating Conditions		Temperature: $0-40^{\circ}$ C, Relative Humidity: $<90\%$ (no dew)		
Drive	Dimensions	232×142×149(mm) (L×W×H)		
Drive	Weight	2.83kg		
IP Rating		IP31		

14